

## The FreeStyle LibreLink app and your Android smartphone


With the FreeStyle LibreLink app,<sup>1</sup> you can scan your FreeStyle Libre 2 sensor with an Android smartphone

**YOU CAN DO IT**  
**WITHOUT LANCETS<sup>2</sup>**




### Downloading the FreeStyle LibreLink app<sup>1</sup>

 Go to **Play Store**


 In the search bar type FreeStyle LibreLink

 Look for FreeStyle LibreLink – UK and **click**

 Click **Install**

 Once downloaded open the app and follow the on-screen instructions to get set-up

### Scanning the FreeStyle Libre 2 sensor with an Android smartphone

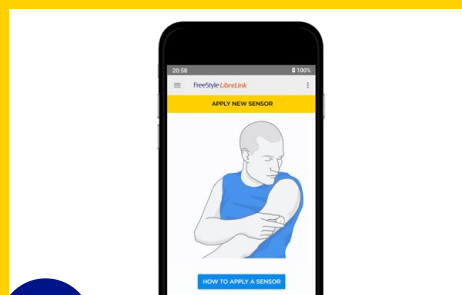

**1** Open the FreeStyle LibreLink app on your Android smartphone



**2** Hold the **back of the Android smartphone** near the sensor and position the NFC antenna over the sensor



**3** Continue holding your smartphone near the sensor until you hear a **second tone** and/or feel a **vibration**. This completes the scan

## ALARM. SCAN. ACT

### Quick Tips

- Remove bulky or metallic phone cases as they can interfere with the Near Field Communication (NFC) signal.
- Do not move the smartphone until you hear the first tone and/or feel a vibration. This indicates your smartphone and sensor have established an NFC connection.

Visit [www.FreeStyleDiabetes.co.uk](http://www.FreeStyleDiabetes.co.uk) for more information

FreeStyle Libre 2   
FLASH GLUCOSE MONITORING SYSTEM


 **Abbott**  
life. to the fullest.®

Images are for illustrative purposes only. Not actual patient or data.

© 2020 Abbott. FreeStyle, Libre, and related brand marks are marks of Abbott. ADC-31516 v1.0 11/20.


# The FreeStyle LibreLink app and your Android smartphone

It's easy to set alarms on your FreeStyle LibreLink app

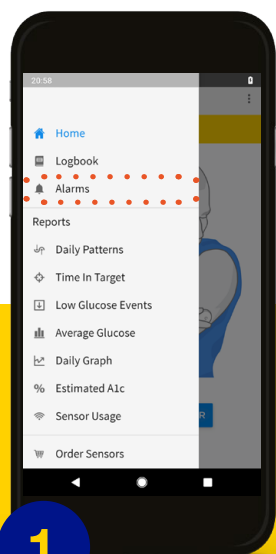



1

Tap Alarms in the menu<sup>3</sup>

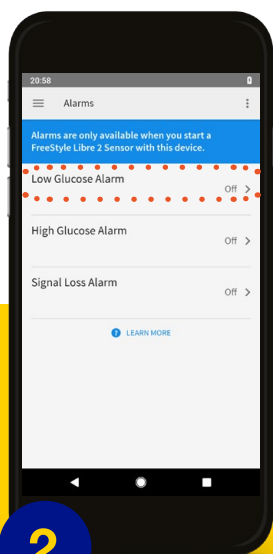


2

Touch **Low Glucose Alarm** and turn on alarm (alarms are off by default)

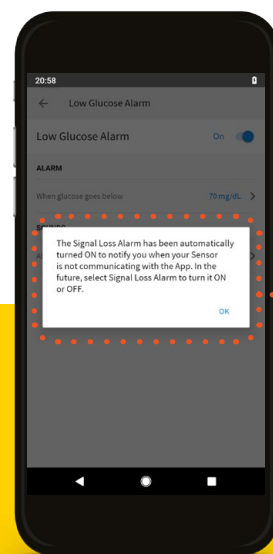
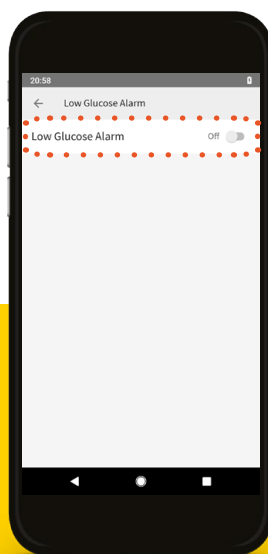


Signal loss alarm is automatically turned on when glucose alarm is turned ON

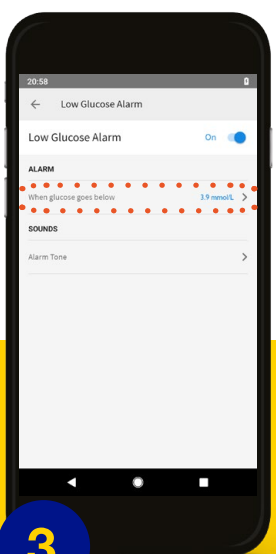


3

Scroll to select **Low Glucose Value**<sup>4</sup>

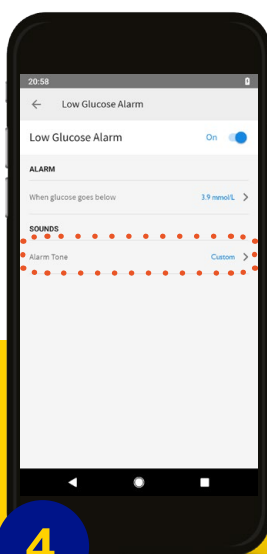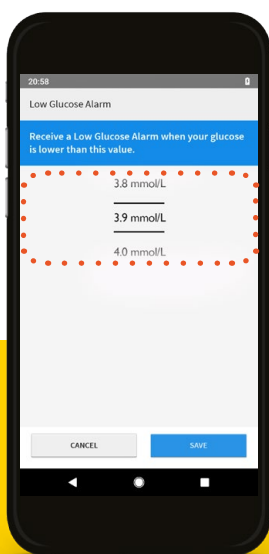

4

Touch **Alarm Tone** and make your tone choice

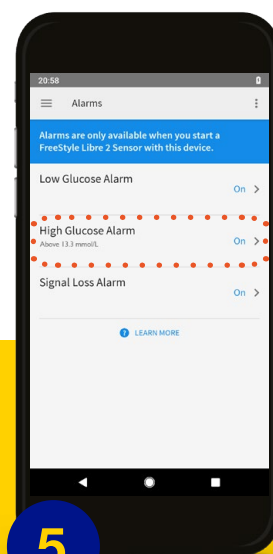

5

Set your **High Glucose Alarm** using the same steps<sup>5</sup>

FreeStyle Libre 2   
FLASH GLUCOSE MONITORING SYSTEM

 **Abbott**  
life. to the fullest.®

Images are for illustrative purposes only. Not actual patient data.

1. The FreeStyle LibreLink app is only compatible with certain mobile devices and operating systems. Please check the website for more information about device compatibility before using the app. Use of FreeStyle LibreLink requires registration with LibreView. 2. Scanning the sensor does not require lancets. 3. Please see the FreeStyle LibreLink User's Manual for complete instructions: [www.diabetescare.abbott/support/manuals/uk.html](http://www.diabetescare.abbott/support/manuals/uk.html) 4. 3.9 mmol/L is the default Low Glucose Alarm level and can be set between 3.3-5.6 mmol/L. 5. 13.3 mmol/L is the default High Glucose Alarm level and can be set between 6.7-22.2 mmol/L.

© 2020 Abbott. FreeStyle, Libre, and related brand marks are marks of Abbott. ADC-31516 v1.0 11/20.